

Configuration Sheet – Cuff Shank

Commission no. / Patient ID:
(no full patient name!)

Reference (Ordernumber, patient ID, ...):

Step 1: What is ordered?

evomwe orthokit (incl. holder)

evomwe solokit (incl. pocket)

Pair of new cuffs (excl. control unit)

right leg

left leg

Control unit (Optional)
Hand (Smartphone)

Fabric color (only one color possible)

● grey ● black

Arm (Watch)

Test supply
(4 weeks)

Continuous supply
after test supply


Continuous supply

Step 2: Recording the measurements (please check)

1. Option: 3D-Scan


Please create a **3D scan** of the leg with the screening electrodes attached.

Important: Please scan with the knee as straight as possible so that both the knee and ankle can be seen. When exporting, make sure that the electrodes are visible (elevated), the scan is complete and has no overlaps.




We accept .obj and .stl files.

2. Option: Measurements with photos

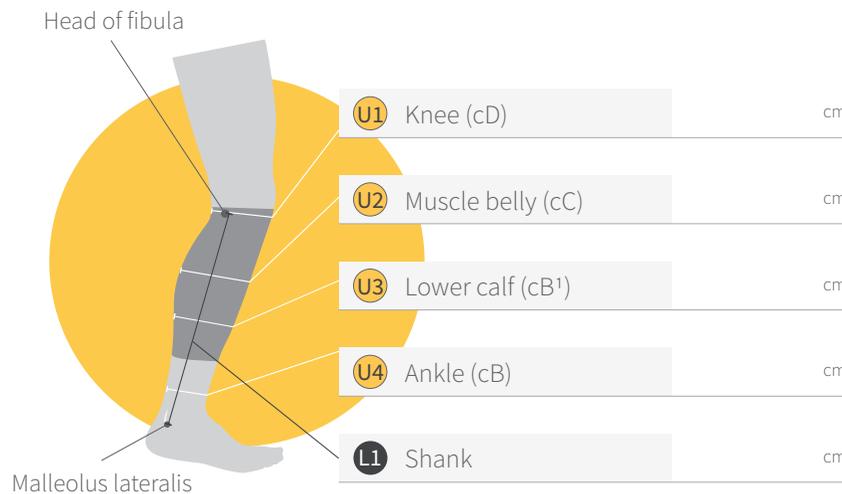


Three photos of the lower leg with corresponding electrodes.

Important: When taking photos, knees and ankles must be visible. Make sure that the camera is at the same height as the legs.

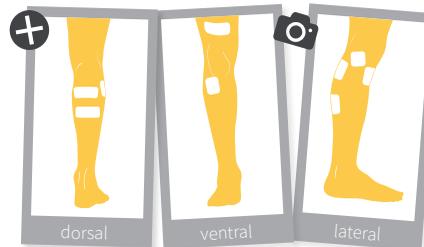


Step 3: Details of the cuff



L2	Cuff length *(Length may vary +/- 2 cm)	Standard (Minimal, all electrodes included) Individual *	cm
T1	Tasche bzw. Kabelaussch	Standard (medial) Individual (please mark on photo or scan)	

R1	Zipper	No	Yes (lateral)*
*Runs from top to bottom over the entire length			
Note: If the cuff length is customized, a zipper cannot always be implemented as we have standard lengths for the zippers.			
S1	Silicone adhesive tape	No	Yes



Please send the **completed** configuration sheet with all images or scan data and any other comments to bestellung@evomotion.de.

Configuration Sheet – Shorts

Commission no. / Patient ID:
(kein vollständige Patient:innen Name!)

Reference (Ordernumber, patient ID ...):

Step 1: What is ordered?

evomove orthokit (incl. holder)

evomove solokit (incl. pocket)

right leg

left leg

female

male

Fabric color (only one color possible)



grey



black

Test supply
(4 Weeks)

Continuous supply
after test supply

Continuous supply

Pair of new shorts (excl. Control unit)


Control unit (Optional)

Hand (Smartphone)

Arm (Watch)

Schritt 2: Measurements (required in any case!)

Circumferences

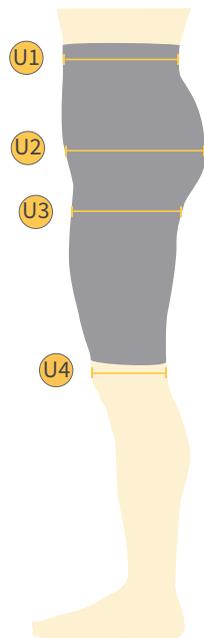

U1

Waist
(midway between the lower costal arch and the iliac crest, level with the navel)

cm

U2

Buttocks
(strongest part buttocks/hips)

cm

Important:

Please measure both legs.

left

right

U3

Thigh
(1cm below crotch)

cm

cm


U4

Knee circumference
(back of the knee)


cm

cm

Lengths

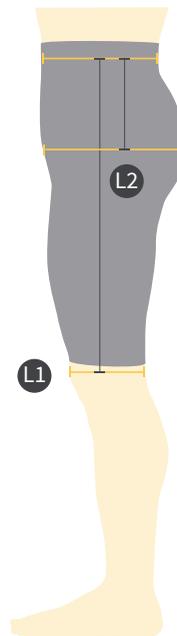

Body dimensions are measured, e.g. using a rubber band to mark the positions U1, U2 and U4.

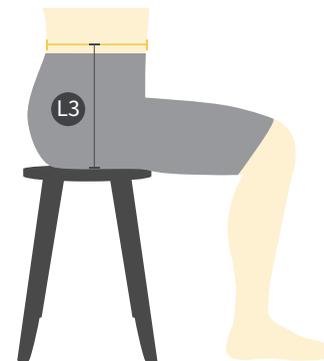

L1

Knee length
(Waist to knee circumference U4)

cm

L2

Buttocks
(Waist – strongest point on the buttocks)

cm

L3

Seat length
(Waist to seat)

Important: The seat should be straight and without cushions.


cm

Body height

cm

Step 3: Detection of the electrode position (Option, please check)

1. Option: 3D-Scan

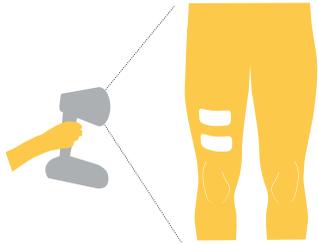

Create a 3D scan using a scanner.

We accept **.obj** and **.stl** files.

Important: When scanning, please make sure that the buttocks and both legs can be seen standing from knee to waist.

2. Option: Photos

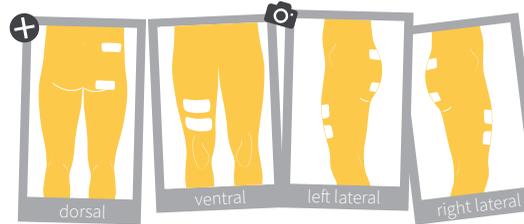



Photo with corresponding electrodes.

Important: When taking the photograph, both legs must be visible from waist to knee while standing. Make sure that the camera is aligned at the same height as the electrodes.

Do not forget: Photograph laterally from both sides.

Step 4: Details of the shorts

1 Cord in waistband	No			
	Yes			
2 Smartphone pocket	none			
	2a right			
	2b left			
3 Zipper (Desired position may be adjusted depending on the electrode position)	No			
	Yes, in the waistband			
	3a right	short	long	
	3b center	short	long	
	3c left	short	long	
	Yes, on the leg			
	3d right	short	long	
	3e left	short	long	

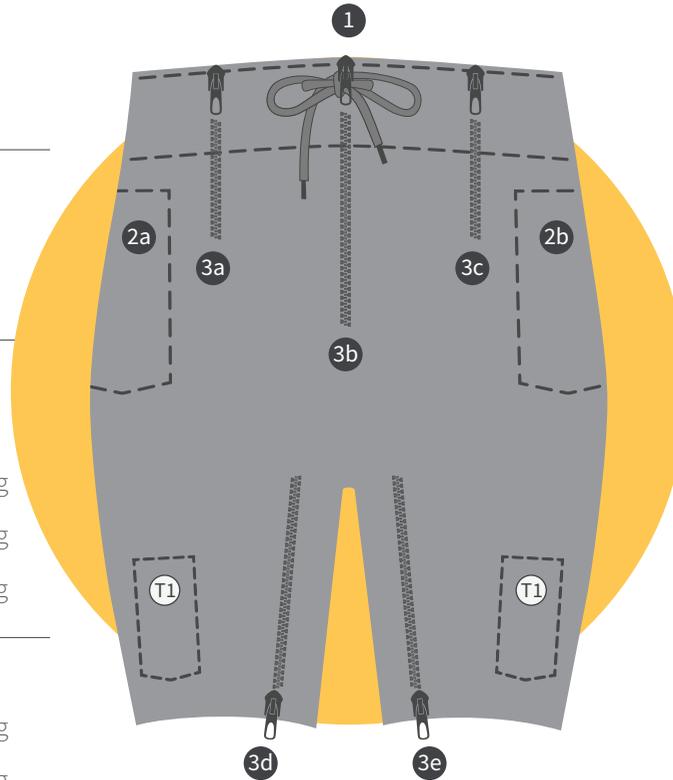

T1 Pocket or cable outlet	Standard (lateral)		
	Individual (please mark on photo or scan)		
Wearing height	Waist shorts	Hipster shorts	

Notes

Please send the **completed** configuration sheet with all images or scan data and any other comments to bestellung@evomotion.de.

Configuration Sheet – Cuff Thigh

Commission no. / Patient ID:
(no full patient name!)

Reference (Ordernumber, patient ID, ...):

Step 1: What is ordered?

evomwe orthokit (incl. holder)

evomwe solokit (incl. pocket)

Pair of new cuffs (excl. control unit)

right leg

left leg

Control unit (Optional)
Hand (Smartphone)

Fabric color (only one color possible)

● grey ● black

Arm (Watch)

Test supply
(4 weeks)

Continuous supply
after test supply


Continuous supply

Step 2: Recording the measurements (please check)

1. Option: 3D-Scan


Please make a **3D scan** of the leg with the screening electrodes attached.

Important: Please scan with the knee stretched as far as possible so that the knee and waist are visible. When exporting, ensure that the electrodes are visible (elevated), the scan is complete and has no overlaps.

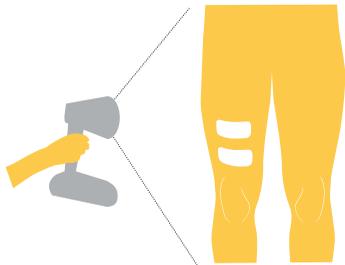


We accept .obj und .stl files.

2. Option: Measurements with photos

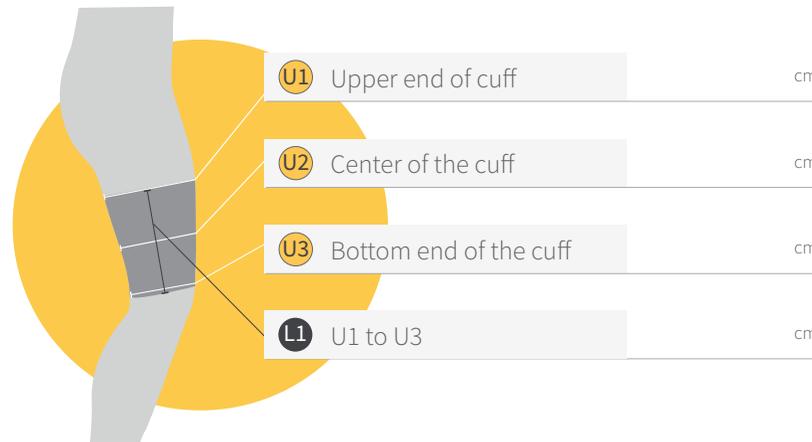


Three photos of the thigh with corresponding electrodes.

Important: When taking pictures, the knee and pelvis must be visible. Make sure that the camera is aligned at the same height as the electrodes.

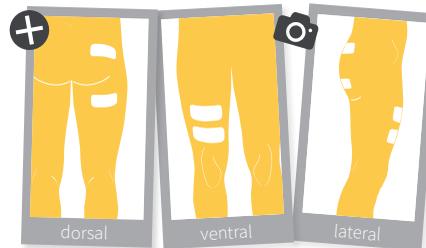

Step 3: Details of the cuff

	L2 Length of cuff *(Length may vary by +/-2 cm)	Standard (Minimal, all electrodes included) Individual *
	T1 Pocket or cable outlet	Standard (lateral) Individual (please mark on photo or scan)
R1 Zipper	No Yes (medial)* *Runs from bottom to top over the entire length Note: A zipper cannot always be used if the cuff is customized in length, as we have standard lengths for the zippers.	
S1 Silicone adhesive tape	No Yes	



Please send the **completed** configuration sheet with all images or scan data and any other comments to bestellung@evomotion.de.